

§ 58.12

40 CFR Ch. I (7–1–23 Edition)

(1) The acceptable concentration range (Rj), $\mu\text{g}/\text{m}^3$ may include values down to 0 $\mu\text{g}/\text{m}^3$.

(2) The minimum number of test sites shall be at least one; however, the number of test sites will generally include all locations within an agency's network with collocated FRMs and FEMs or ARMs.

(3) The minimum number of methods shall include at least one FRM and at least one FEM or ARM.

(4) Since multiple FRMs and FEMs may not be present at each site; the precision statistic requirement does not apply, even if precision data are available.

(5) All seasons must be covered with no more than thirty-six consecutive months of data in total aggregated together.

(6) The key statistical metric to include in an assessment is the bias (both additive and multiplicative) of the $\text{PM}_{2.5}$ continuous FEM(s) compared to a collocated FRM(s). Correlation is required to be reported in the assessment, but failure to meet the correlation criteria, by itself, is not cause to exclude data from a continuous FEM monitor.

[71 FR 61298, Oct. 17, 2006, as amended at 78 FR 3282, Jan. 15, 2013; 80 FR 65466, Oct. 26, 2015; 81 FR 17279, Mar. 28, 2016]

§ 58.12 Operating schedules.

State and local governments shall collect ambient air quality data at any SLAMS station on the following operational schedules:

(a) For continuous analyzers, consecutive hourly averages must be collected except during:

(1) Periods of routine maintenance,

(2) Periods of instrument calibration, or

(3) Periods or monitoring seasons exempted by the Regional Administrator.

(b) For Pb manual methods, at least one 24-hour sample must be collected every 6 days except during periods or seasons exempted by the Regional Administrator.

(c) For PAMS VOC samplers, samples must be collected as specified in section 5 of appendix D to this part. Area-specific PAMS operating schedules must be included as part of the PAMS

network description and must be approved by the Regional Administrator.

(d) For manual $\text{PM}_{2.5}$ samplers:

(1)(i) Manual $\text{PM}_{2.5}$ samplers at required SLAMS stations without a collocated continuously operating $\text{PM}_{2.5}$ monitor must operate on at least a 1-in-3 day schedule unless a waiver for an alternative schedule has been approved per paragraph (d)(1)(ii) of this section.

(ii) For SLAMS $\text{PM}_{2.5}$ sites with both manual and continuous $\text{PM}_{2.5}$ monitors operating, the monitoring agency may request approval for a reduction to 1-in-6 day $\text{PM}_{2.5}$ sampling or for seasonal sampling from the EPA Regional Administrator. Other requests for a reduction to 1-in-6 day $\text{PM}_{2.5}$ sampling or for seasonal sampling may be approved on a case-by-case basis. The EPA Regional Administrator may grant sampling frequency reductions after consideration of factors (including but not limited to the historical $\text{PM}_{2.5}$ data quality assessments, the location of current $\text{PM}_{2.5}$ design value sites, and their regulatory data needs) if the Regional Administrator determines that the reduction in sampling frequency will not compromise data needed for implementation of the NAAQS. Required SLAMS stations whose measurements determine the design value for their area and that are within ± 10 percent of the annual NAAQS, and all required sites where one or more 24-hour values have exceeded the 24-hour NAAQS each year for a consecutive period of at least 3 years are required to maintain at least a 1-in-3 day sampling frequency until the design value no longer meets these criteria for 3 consecutive years. A continuously operating FEM or ARM $\text{PM}_{2.5}$ monitor satisfies this requirement unless it is identified in the monitoring agency's annual monitoring network plan as not appropriate for comparison to the NAAQS and the EPA Regional Administrator has approved that the data from that monitor may be excluded from comparison to the NAAQS.

(iii) Required SLAMS stations whose measurements determine the 24-hour design value for their area and whose data are within ± 5 percent of the level of the 24-hour $\text{PM}_{2.5}$ NAAQS must have an FRM or FEM operate on a daily schedule if that area's design value for

the annual NAAQS is less than the level of the annual $PM_{2.5}$ standard. A continuously operating FEM or ARM $PM_{2.5}$ monitor satisfies this requirement unless it is identified in the monitoring agency's annual monitoring network plan as not appropriate for comparison to the NAAQS and the EPA Regional Administrator has approved that the data from that monitor may be excluded from comparison to the NAAQS. The daily schedule must be maintained until the referenced design value no longer meets these criteria for 3 consecutive years.

(iv) Changes in sampling frequency attributable to changes in design values shall be implemented no later than January 1 of the calendar year following the certification of such data as described in § 58.15.

(2) Manual $PM_{2.5}$ samplers at NCore stations and required regional background and regional transport sites must operate on at least a 1-in-3 day sampling frequency.

(3) Manual $PM_{2.5}$ speciation samplers at STN stations must operate on at least a 1-in-3 day sampling frequency unless a reduction in sampling frequency has been approved by the EPA Administrator based on factors such as area's design value, the role of the particular site in national health studies, the correlation of the site's species data with nearby sites, and presence of other leveraged measurements.

(e) For PM_{10} samplers, a 24-hour sample must be taken from midnight to midnight (local standard time) to ensure national consistency. The minimum monitoring schedule for the site in the area of expected maximum concentration shall be based on the relative level of that monitoring site concentration with respect to the 24-hour standard as illustrated in Figure 1. If the operating agency demonstrates by monitoring data that during certain periods of the year conditions preclude violation of the PM_{10} 24-hour standard, the increased sampling frequency for those periods or seasons may be ex-

empted by the Regional Administrator and permitted to revert back to once in six days. The minimum sampling schedule for all other sites in the area remains once every six days. No less frequently than as part of each 5-year network assessment, the most recent year of data must be considered to estimate the air quality status at the site near the area of maximum concentration. Statistical models such as analysis of concentration frequency distributions as described in "Guideline for the Interpretation of Ozone Air Quality Standards," EPA-450/479-003, U.S. Environmental Protection Agency, Research Triangle Park, NC, January 1979, should be used. Adjustments to the monitoring schedule must be made on the basis of the 5-year network assessment. The site having the highest concentration in the most current year must be given first consideration when selecting the site for the more frequent sampling schedule. Other factors such as major change in sources of PM_{10} emissions or in sampling site characteristics could influence the location of the expected maximum concentration site. Also, the use of the most recent 3 years of data might, in some cases, be justified in order to provide a more representative database from which to estimate current air quality status and to provide stability to the network. This multiyear consideration reduces the possibility of an anomalous year biasing a site selected for accelerated sampling. If the maximum concentration site based on the most current year is not selected for the more frequent operating schedule, documentation of the justification for selection of an alternative site must be submitted to the Regional Office for approval during the 5-year network assessment process. Minimum data completeness criteria, number of years of data and sampling frequency for judging attainment of the NAAQS are discussed in appendix K of part 50 of this chapter.

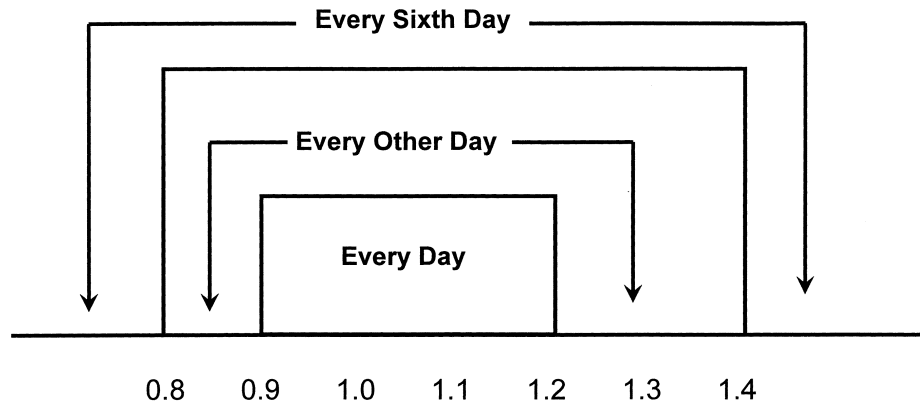


Figure 1 – Ratio to Standard

(f) For manual $PM_{10-2.5}$ samplers:

(1) Manual $PM_{10-2.5}$ samplers at NCore stations must operate on at least a 1-in-3 day schedule at sites without a collocated continuously operating federal equivalent $PM_{10-2.5}$ method that has been designated in accordance with part 53 of this chapter.

(2) [Reserved]

(g) For continuous SO_2 analyzers, the maximum 5-minute block average concentration of the twelve 5-minute blocks in each hour must be collected except as noted in § 58.12 (a).

[71 FR 61298, Oct. 17, 2006, as amended at 72 FR 32210, June 12, 2007; 75 FR 35601, June 22, 2010; 78 FR 3282, Jan. 15, 2013; 81 FR 17279, Mar. 28, 2016]

§ 58.13 Monitoring network completion.

(a) The network of NCore multi-pollutant sites must be physically established no later than January 1, 2011, and at that time, operating under all of the requirements of this part, including the requirements of appendices A, C, D, E, and G to this part. NCore sites required to conduct Pb monitoring as required under 40 CFR part 58 appendix D paragraph 3(b), or approved alternative non-source-oriented Pb monitoring sites, shall begin Pb monitoring in accordance with all of the requirements of this part, including the requirements of appendices A, C, D, E,

and G to this part no later than December 27, 2011.

(b) Notwithstanding specific dates included in this part, beginning January 1, 2008, when existing networks are not in conformance with the minimum number of required monitors specified in this part, additional required monitors must be identified in the next applicable annual monitoring network plan, with monitoring operation beginning by January 1 of the following year. To allow sufficient time to prepare and comment on Annual Monitoring Network Plans, only monitoring requirements effective 120 days prior to the required submission date of the plan (i.e., 120 days prior to July 1 of each year) shall be included in that year's annual monitoring network plan.

(c) The NO_2 monitors required under Appendix D, section 4.3 of this part must be physically established and operating under all of the requirements of this part, including the requirements of appendices A, C, D, and E to this part, no later than:

(1) January 1, 2013, for area-wide NO_2 monitors required in Appendix D, section 4.3.3;

(2) January 1, 2013, for NO_2 monitors intended to characterize vulnerable and susceptible populations that are required in Appendix D, section 4.3.4;